

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 11:02

Date of Inspection: 02/07/2022

Serial Number: 80-003935
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08g/210L Test (g/210L) Lot#:_____ Exp:_____	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____
0.000				
0.000				
0.000				

Number of Simulators Used: 5

Remarks: TEST RESTARTED. ENTERING 0.05 LOT/EXP HIT "N" IN ERROR. RE-TEST WITH IN COMPLIANCE.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

02/07/2022
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 11:53

Date of Inspection: 02/07/2022

Serial Number: 80-003935
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.049	0.079	0.198	0.080
0.000	0.049	0.079	0.199	0.080
0.000	0.049	0.079	0.199	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

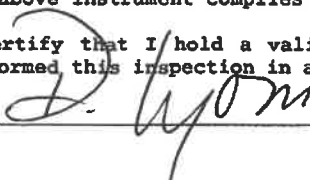

DANIEL E LYONS

Signature and Printed Name

02/07/2022
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 15:04

Date of Inspection: 05/25/2022

Serial Number: 80-003935

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.054 / 0.053	0.080	0.214 / 0.210	0.082
0.000	0.060 / 0.050	0.080	0.209 / 0.210	0.081
0.000	INT / 0.054	0.076	0.207 / 0.206	0.084

Number of Simulators Used: 5

Remarks:

05: Int Detect. 20: Control Outside Tolerance.

05. RE-SET INST, RE-TESTED AFTER AIR OUT w/ OPEN DOOR
20. CONNECTION NOT COMPLETED / RE-SET / RETESTED

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D E LTONS

DANIEL E LTONS

Signature and Printed Name

05/25/2022
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 11:44

Date of Inspection: 06/13/2022

Serial Number: 80-003935
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____
0.000	0.053	0.085	0.211 / 0.210	
0.000	0.054	0.085	0.213 / 0.212	
0.000	0.053	0.085	0.207 / 0.211	

Number of Simulators Used: 5


Remarks:

20: Control Outside Tolerance, Control Outside Tolerance. Non-compliance:OUT TOL .20 SOLUTION.

CHANGED OUT .20 SOLUTION RE-TESTED

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

06/13/2022
Date

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 11:01

Date of Inspection: 06/13/2022

Serial Number: 80-003935
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#: 202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#: 202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:
0.000	0.053	0.083	0.214 / 0.211	
0.000	0.052	0.084	0.212 / 0.209	
0.000	0.052	0.084	0.210 / 0.211	

Number of Simulators Used: 5


Remarks:

20: Control Outside Tolerance, Control Outside Tolerance.

w/ NEW SOLUTION / READ HIGH
REMOVED FROM SVC / SENT FOR
REVIEW / REPAIR

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

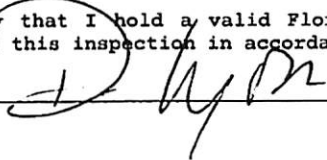

DANIEL E LYONS

Signature and Printed Name

06/13/2022
Date